


QUICK GUIDE VIO® 200 D


 This quick guide is no substitute for briefing and user manual. This quick guide does not include any safety notes. Make yourself familiar with the safety notes in the user manuals.

Necessary operating steps


1 Switch on the device

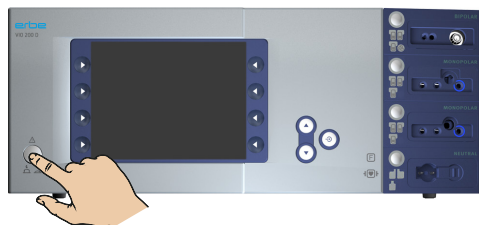


2 Select program

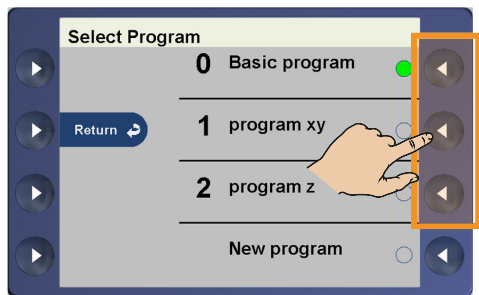

3 Check settings

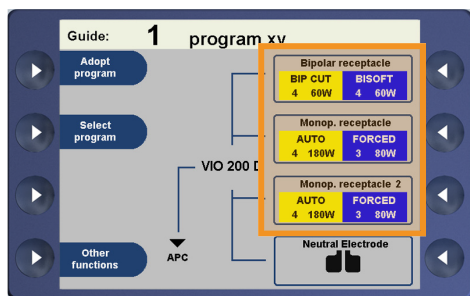

4 Apply and connect return electrode

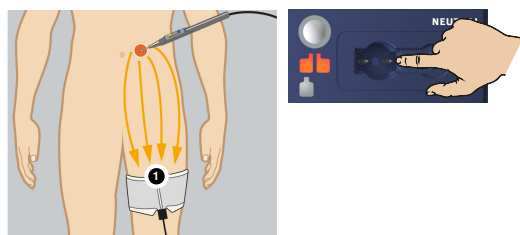

The long edge of the return electrode (1) must point to the operating field.


5 Monitor return electrode



If the red return electrode symbol lights up, check the following:


- Is the return electrode correctly connected to the device?
- Does the long edge of the return electrode point to the operating field?
- Does the return electrode have sufficient contact to the skin?

6 Connect instruments

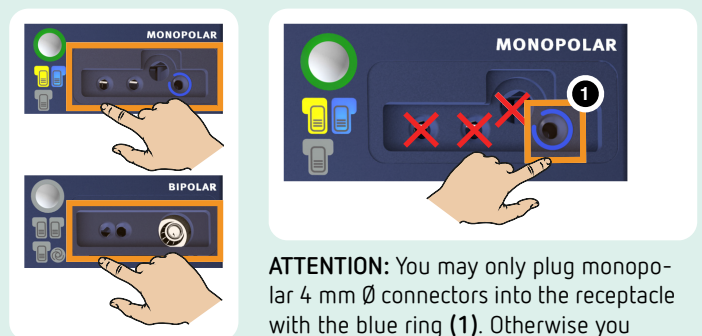



ATTENTION: You may only plug monopolar 4 mm Ø connectors into the receptacle with the blue ring (1). Otherwise you damage the device.

7 For APC applications, open argon bottle



Optional operating steps



8 Changing mode

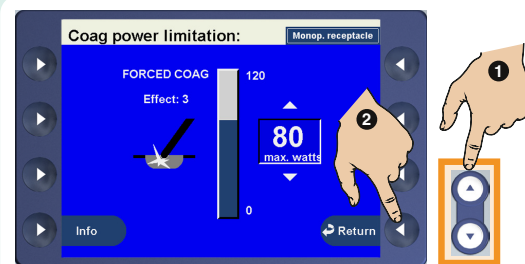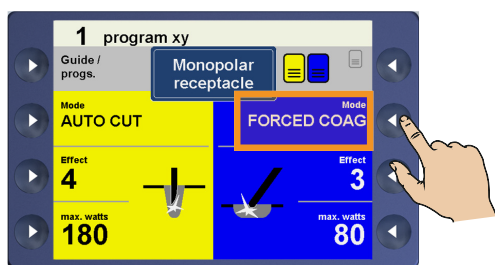


11 Selecting the focus view of a receptacle



9 Changing effect

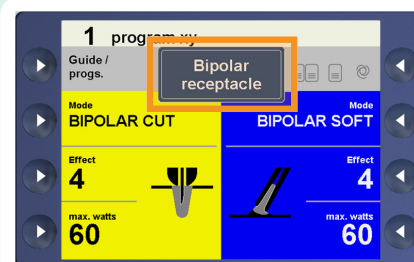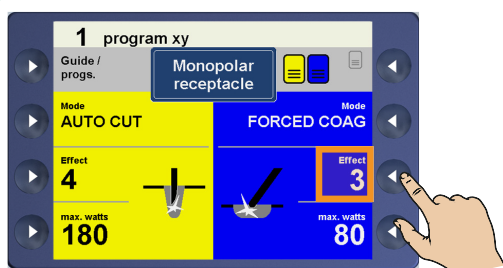

12 Allocating foot switch or AUTO START

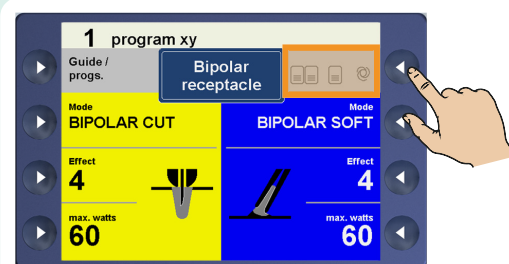

10 Changing power limit

